

Fluke TC03A / TC03A PRO

Thermal Camera for Smart Device

Users Guide

LIMITED WARRANTY AND LIMITATION OF LIABILITY

Each Fluke product is warranted to be free from defects in material and workmanship under normal use and service. The warranty period is two years and begins on the date of shipment. Parts, product repairs, and services are warranted for 90 days. This warranty extends only to the original buyer or end-user customer of a Fluke authorized reseller, and does not apply to fuses, disposable batteries, or to any product which, in Fluke's opinion, has been misused, altered, neglected, contaminated, or damaged by accident or abnormal conditions of operation or handling. Fluke warrants that software will operate substantially in accordance with its functional specifications for 90 days and that it has been properly recorded on non-defective media. Fluke does not warrant that software will be error free or operate without interruption.

Fluke authorized resellers shall extend this warranty on new and unused products to end-user customers only but have no authority to extend a greater or different warranty on behalf of Fluke. Warranty support is available only if product is purchased through a Fluke authorized sales outlet or Buyer has paid the applicable international price. Fluke reserves the right to invoice Buyer for importation costs of repair/replacement parts when product purchased in one country is submitted for repair in another country. Fluke's warranty obligation is limited, at Fluke's option, to refund of the purchase price, free of charge repair, or replacement of a defective product which is returned to a Fluke authorized service center within the warranty period.

To obtain warranty service, contact your nearest Fluke authorized service center to obtain return authorization information, then send the product to that service center, with a description of the difficulty, postage and insurance prepaid (FOB Destination). Fluke assumes no risk for damage in transit. Following warranty repair, the product will be returned to Buyer, transportation prepaid (FOB Destination). If Fluke determines that failure was caused by neglect, misuse, contamination, alteration, accident, or abnormal condition of operation or handling, including overvoltage failures caused by use outside the product's specified rating, or normal wear and tear of mechanical components, Fluke will provide an estimate of repair costs and obtain authorization before commencing the work. Following repair, the product will be returned to the Buyer transportation prepaid and the Buyer will be billed for the repair and return transportation charges (FOB Shipping Point).

THIS WARRANTY IS BUYER'S SOLE AND EXCLUSIVE REMEDY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. FLUKE SHALL NOT BE LIABLE FOR ANY SPECIAL, INDIRECT, INCIDENTAL OR CONSEQUENTIAL DAMAGES OR LOSSES, INCLUDING LOSS OF DATA, ARISING FROM ANY CAUSE OR THEORY.

Since some countries or states do not allow limitation of the term of an implied warranty, or exclusion or limitation of incidental or consequential damages, the limitations and exclusions of this warranty may not apply to every buyer. If any provision of this Warranty is held invalid or unenforceable by a court or other decision-maker of competent jurisdiction, such holding will not affect the validity or enforceability of any other provision.

Fluke Corporation
6920 Seaway Blvd.
Everett, WA 98203
U.S.A.

Fluke Europe B.V
PO Box 1186
5602 BD EINDHOVEN
The Netherlands

Introduction

The TC03A / TC03A PRO (the Product or Camera) is a Thermal Camera that attaches to a smart device. You can get thermal images and conduct non-contact temperature measurement from the Camera on your smart devices using the iSee™ App. Use the Product for many applications, such as equipment troubleshooting, preventive and predictive maintenance, buildings diagnostics, and more.

Contact Fluke

Fluke Corporation operates worldwide. For local contact information, go to our website: www.fluke.com.

To register your product, view, print, or download the latest manual or manual supplement, go to our website.


+1-425-446-5500 fluke-info@fluke.com

Main Features

- Take, edit, and share infrared pictures.
- Take and share infrared video.
- Non-contact temperature measurement up to 550 °C (1022 °F).
- Field monitoring (interval captures).
- Customized palette.
- Analyze dot, line, and zone temperature.
- Alarm for the area over or below preset temperature range and take photo or video automatically
- 3 phase measurement profile with delta temperature calculation.
- Infrared report generation for one or several infrared pictures.

Product Diagram

Table 1. Product Diagram

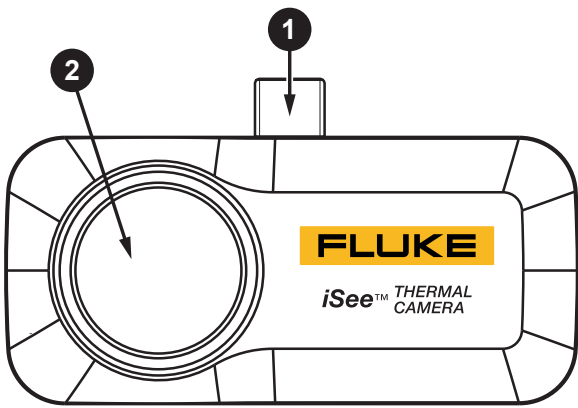	
Item	Description
①	Type-C connector
②	Infrared Lens
<i>Note: This product does not include Smart devices.</i>	

Operating Instruction

- The Product requires a smart device such as a smartphone. Download and install Fluke iSee™ App on your smart device. To download the software. See [Figure 1](#).


Required Equipment

- The Fluke iSee App™ supports Android 12.0 / HarmonyOS 2.0 and above versions. Enable the OTG feature of your smartphone.
- The Product does not contain a battery. The Product is powered by the smart devices.
- To prevent damage to the connector and USB port, be gentle when you plug and unplug the Product.
- For more accurate measurements, do a manual nonuniformity correction (usually called NUC or shutter) before you take an infrared picture.

To use the Product

- Plug in the product to your smart devices. See [Figure 2](#).
- Run the App (When the Product is plugged in, the App will auto pop-up if it is already installed on your smart devices. See [Figure 3](#).)
- To make an accurate measurement, you must properly set the measuring parameters. For example emissivity, measuring distance, background temperature, and others. Refer to the help file in the App. See [Figure 4](#).

To provide an optimal image, the Camera automatically refreshes the image periodically by a internal mechanical shutter, it makes a clicking sound when it activates and the image might freeze briefly. You can also use the iSee App to manually activate the shutter.

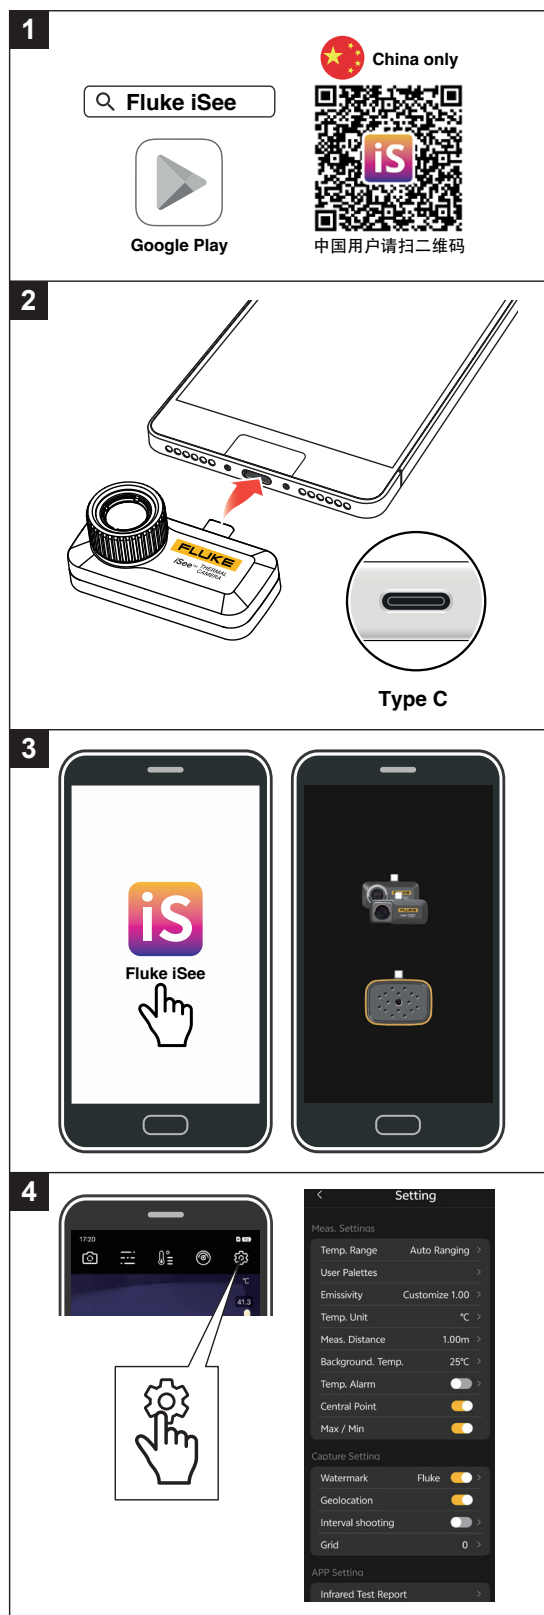

Cleaning the Lens

Always keep the lens clean. A clean lens is important to good pictures and accurate measurements. To clean the lens:

1. Lightly blow off loose particles with canned air or a small squeeze bellows.
2. Gently brush off any remaining particles with a soft camel hair brush or a soft lens tissue.
3. Clean remaining dirt using a cotton swab or soft lens tissue dampened in distilled water. Do not scratch the surface.
4. For fingerprints or other grease, apply Ethanol or denatured alcohol to the lens. Wipe gently with a soft, clean cloth until you see colors on the surface, then allow to air dry.
5. If silicones (used in hand creams) get on the window, gently wipe the surface with Hexane. Allow to air dry.

Specifications

General Specifications

Connector	Type-C
Operating Temperature	0 °C to +40 °C (32 °F to 104 °F)
Storage Temperature	-30 °C to +60 °C (-22 °F to 140 °F)
Operating Humidity	10% to 90% RH, Non condensing (<10°C)
Power Consumption	700 mW (Typical)
Ingress Protection (IP) Rating	IEC 60529: IP54 (with type-C connector covered)
Operating Altitude	2000 m
Storage Altitude	12000 m
Size (L x W x H)	60 mm x 36 mm x 28 mm
Weight	55 g
Electromagnetic Compatibility (EMC)	
International	IEC 61326-1: Portable Electromagnetic Environment CISPR 11: Group 1, Class A <i>Group 1: Equipment has intentionally generated and/or uses conductively-coupled radio frequency energy that is necessary for the internal function of the equipment itself.</i> <i>Class A: Equipment is suitable for use in all establishments other than domestic and those directly connected to a lowvoltage power supply network that supplies buildings used for domestic purposes. There may be potential difficulties in ensuring electromagnetic compatibility in other environments due to conducted and radiated disturbances.</i> <i>Caution: This equipment is not intended for use in residential environments and may not provide adequate protection to radio reception in such environments.</i>
Korea (KCC)	Class A equipment (Industrial Broadcast & Communications Equipment) <i>Class A: Equipment meets requirements for industrial electromagnetic wave equipment and the seller or user should take notice of it. This equipment is intended for use in business environments and not to be used in homes.</i>
USA (FCC)	47 CFR 15 subpart B. This product is considered an exempt device per clause 15.103.

Optical Performance

Image Resolution	384 x 288
Super Resolution	768 x 576
Pixel Size	12 μm
Measuring Range	-20 °C to 150 °C, 100 °C to 550 °C (-4 °F to 302 °F, 212 °F to 1022 °F)
Accuracy	$\pm 2\%$ of reading / ± 2 °C (3.6 °F), whichever is greater (at 23 ± 5 °C, 73 ± 9 °F ambient)
Distance	0.25 m to 20 m ^[1]
Frame Rate	TC03A: 9 Hz / 25 Hz TC03A PRO: 50 Hz
Warm Up	15 minute
Focus	Fixed 10.5 mm
Nonuniformity correction (NUC)	Auto or manual
NETD	TC03A: 50 mK TC03A PRO: 45 mK
Spectral Range	8 to 14 μm
Field of View (H x V)	25° x 19°
Spatial Resolution (IFOV)	1.14 mrad
^[1] Accuracy is unspecified when measuring distance over 10m.	